

1 **Supplemental information**

2 The new dilution system almost exclusively consists of stainless steel parts (Figure S1). Low
3 pressures (50 to 300 mbar, measured with a PX764-005GI Industrial Pressure Transmitter
4 from Omega, UK) of pure gases can be trapped inside two sample loops (obtained from VICI
5 AG International, Switzerland) which have calibrated volumes (used here: 2.00 ± 0.1 ml). The
6 loop is connected to a 1/16" six-port two-position Valco valve (with Valcon E rotor, also from
7 VICI) which is used to isolate the sample loop after filling. The system is then filled with
8 OFN to about 2 bars (measured with a Swagelok S Model Transducer) and evacuated to about
9 1 mbar (measured with a TPR-280 gauge from Pfeiffer Vacuum, Germany) using a XDS-10
10 scroll pump from Edwards, UK. This procedure is repeated 10 times to remove residual
11 compound from the system. It is then again filled with OFN and the valve leading to an
12 aluminium drum (filled with OFN at atmospheric pressure) with a volume of 99.7 litres is
13 opened. When a constant flow (here: about 300 ml/min measured with a Tylan 260 Series
14 MFC from Millipore, USA) into the drum has established the sample loop with the pure gas is
15 switched into this flow and flushed for about 4 minutes. The drum is then closed and an inside
16 fan turned on for 30 minutes to create a uniform gas mixture. As an evaluation of this dilution
17 system we chose to add a gas with known mixing ratios (here: CF_2Cl_2 as obtained from
18 Fluorochem Ltd., UK) as internal reference. All first steps of the dilution procedure were
19 repeated for this purpose. After additional 30 minutes of mixing the drum is reconnected to a
20 second similar system which contained similar parts i.e. a volume-calibrated sample loop
21 (here: 10.00 ± 0.5 ml) connected to another six port Valco valve and a Pfeiffer APR-262
22 Pressure Gauge (range: 2000 mbar). The second dilution step is carried out in a similar
23 manner by taking an aliquot out of the first dilution drum, cleaning the exposed gas lines with
24 OFN (10 times) and flushing it into a second 99.7 litre aluminium drum. After another 30

1 minutes of mixing this drum was measured against a tertiary compressed air standard filled
2 and calibrated in 2006 by the Global Monitoring Division (GMD) of the National Oceanic
3 Atmospheric Administration - Earth System Research Laboratory (NOAA-ESRL, USA).
4 CF₂Cl₂ dilutions containing 136, 186 and 192 ppt were prepared. Both drums were flushed for
5 at least 3 hours with OFN (flow of about 10 l/min) before reusing them. All mixing ratios
6 agreed with those derived via the NOAA calibration value (2001 scale) within 1.3 %. It
7 should be noted, that both the NOAA-scale and our mixing ratios are reported as dry air mole
8 fractions. NOAA values are, however, derived gravimetrically whereas our values depend on
9 a volume measurement and thus on the ideal gas law. Comparing these values includes the
10 assumption, that intermolecular interactions are negligible. For the pressures, temperatures
11 (between 80 and 130 mbar at 80 °C) and compounds used the systematic errors introduced by
12 assuming ideal gas conditions are between 0.09 and 0.20 % (calculated by using virial
13 coefficients from Duan et al., 2001 for HFC-227ea and from Schramm et al., 1992 for
14 CF₂Cl₂). We applied the respective corrections in order to report dry air mole fractions but
15 also note that these errors are far smaller than the accuracy and precision of our
16 determinations here. Eq. S1 summarises the calculation of mixing ratios for the first dilution
17 step.

18

$$19 \quad \chi_i = f_{v,i} \left[\frac{f_{p,i} p_i V_S}{RT_O} \bigg/ \frac{p_D V_D}{RT_D} \right] \quad (S1)$$

20 χ_i - Mixing ratio of compound i in drum

21 $f_{v,i}$, $f_{p,i}$ - Correction factors for virial coefficients and purity of the compound

22 p_i , p_D - pressures in sample loop and drum

1 V_S, V_D - Volumes of sample loop and drum

2 T_O, T_D - Temperatures in oven and drum

3

4 The three prepared dilutions contained CF_2Cl_2 and HFC-227ea (97%, obtained from Apollo
5 Scientific, UK) with mixing ratios of 144, 194 and 222 ppt for the latter. The mixing ratio
6 assigned to the NOAA standard via these dilutions was (0.3542 ± 0.0064) ppt. As we were
7 bridging almost three orders of magnitude with this calibration we needed to make sure that
8 the response behaviour of the whole analytical procedure including pre-concentration,
9 separation, detection and retrieval was linear over that range. Thus, different amounts of the
10 same NOAA standard (49, 102, 194, 199, 224 and 301 ml) were pre-concentrated and
11 measured. The response behaviour was checked and found to be linear within the average 1σ
12 standard deviation of the standard not only for HFC-227ea but also for CF_2Cl_2 (534.1 ppt in
13 standard), $\text{CF}_2\text{ClCFCl}_2$ (79.8 ppt, NOAA 2002 calibration scale), SF_6 (5.95 ppt, NOAA
14 2006), and CF_3Br (3.0 ppt, NOAA 2006). Therefore we conclude that the analytical system
15 responds linearly within the given range. By propagating the average 1σ standard deviation
16 uncertainty of the dilutions (1.8 %), of the NOAA standard (1.4 %), the sample loop volume
17 (5% for each of them), the drum volume (0.5 %) and the pressure gauge (less than 0.5 %) we
18 estimate the sum of our uncertainties to be about 14 %. However, taking into account the
19 good agreement of the CFC-12 dilutions with the NOAA scale as well as the small variability
20 between calibrations for HFC-227ea (< 4 %) the total scale uncertainty is likely to be 5 % at
21 the most.

22 The complete dilution system was evaluated for blank levels which were found to be
23 consistently about 2.5 ppt for CFC-12 and 0.025 ppt for HFC-227ea. These were taken into
24 account for the mixing ratio calculation but are negligible especially for HFC-227ea. Blank

1 levels of the pre-concentration/GC-MS system were negligible for CFC-12 and about 0.001
2 ppt for HFC-227ea.

3

4 **References**

5 Duan, Y. Y., Shi, L., Zhu, M. S., Han, L. Z., and Zhang, C.: Thermodynamic Properties of
6 1,1,1,2,3,3,3-Heptafluoropropane, *Int. J. Thermophys.*, 22 (5), 1463-1474, 2001.

7

8 Schramm, B., Hauck, J., and Kern, L.: Measurements of the second virial coefficients of some
9 new chlorofluorocarbons and of their binary mixtures at temperatures in the range from 296 K
10 to 475 K, *Ber. Bunsen. Phys. Chem.*, 96, 745-750, 1992.

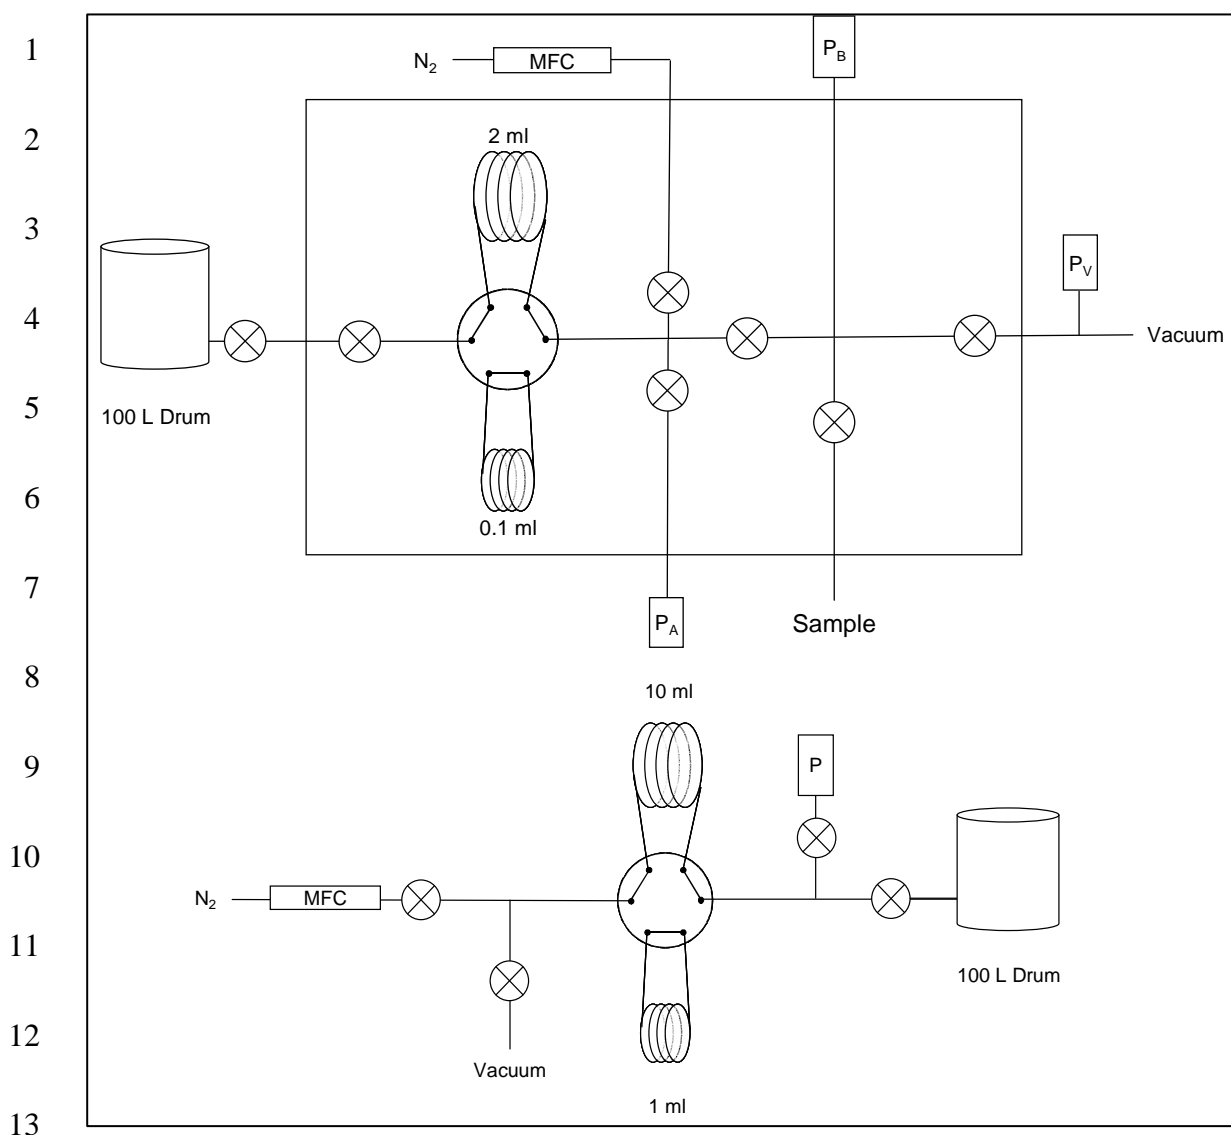


Figure S1. Layout of the dilution system used to calibrate HFC-227ea. At stage one (upper part) a sample loop is filled with the pure compound at low pressures which are monitored by a high accuracy pressure gauge P_A . Low accuracy pressure gauges are used to avoid over-pressurisation of the system during cleaning with N_2 (P_B) and to monitor the vacuum (P_V). After filling, the sample loop is isolated and the rest of the system cleaned. Then the contents of the sample loop are flushed into a 100 litre drum which is filled with N_2 at atmospheric pressure while maintaining the flow with a mass flow controller (MFC). Most of the system used for this dilution step is heated (box) to achieve quantitative transport into the drum. For

- 1 the second step an aliquot is taken out of the first drum and diluted into a second by carrying
- 2 out a similar procedure (lower part).
- 3