



Supplement of

Technical note: Characterization of a single-beam gradient force aerosol optical tweezer for droplet trapping, phase transition monitoring, and morphology studies

Xiangyu Pei et al.

Correspondence to: Zhibin Wang (wangzhibin@zju.edu.cn)

The copyright of individual parts of the supplement might differ from the article licence.

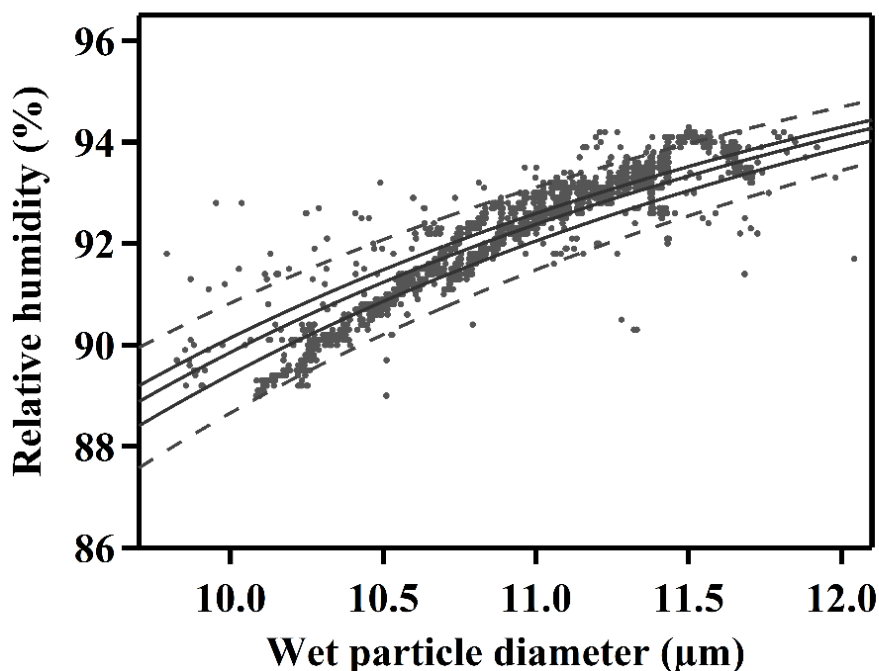


Figure S1. Comparison between experimental measurements and theoretical calculations of the relationship between wet particle diameter and relative humidity at higher RH compare to Figure 4(a). The lines represent Köhler curves calculated for particles with different diameters: 4.10 μm , 4.20 μm , 4.24 μm , 4.30 μm , and 4.40 μm from left to right, respectively.

Figure S1 shows the comparison between experimental measurements and theoretical calculations of the relationship between wet particle diameter and relative humidity of another droplet at higher RH compare to Figure 4(a). In Figure S1, measured values are generally consistent with the theoretical calculations. In both Figure S1 and Figure 4(a), the RH was measured with the RH sensor at the exit of the chamber, while wet particle diameters were retrieved from the spectra with the Mie fitting program MRFIT. The typical and maximal tolerances for the RH sensor are $\pm 1.5\%$ and $\pm 1.8\%$ when RH is lower than 80%, respectively. When RH increases from 80% to 100%, the typical and maximal tolerances for the RH sensor also increase linearly until $\pm 2\%$ and $\pm 3\%$, respectively (Sensirion SHT85 datasheet). As a result, the measured RH values at high RH have more uncertainty. In Figure 4(a) and Figure S1, we think that the experiment deviation from theory is due to the increasing measurement uncertainty of the RH sensor. In Figure 4, when RH is higher than 85% during this experiment, the wet particle diameters retrieved from the program MRFIT represents hysteresis. For example, when RH is about 86%, the wet particle diameters are in the range of 11.8-12.2 μm , and the range (0.4 μm) is much larger than the value ($\sim 0.01 \mu\text{m}$) when RH is lower than 86%, which is shown in Figure 4(b). This hysteresis can be explained by that when RH is high, more WGMs peaks represent in each spectrum, the assignment of WGMs labels may have differences since different combination of WGMs labels

can lead to the same WGM positions. In Figure S1, the RH values are in the higher range of 88-94% compare to Figure 4(a), which means the measurement uncertainty of the RH sensor is even higher. Considering all the factors above, we still think that the measured values and theoretical values are generally consistent.

References

Sensirion SHT 85 datasheet,
https://sensirion.com/media/documents/4B40CEF3/61642381/Sensirion_Humidity_Sensors_SHT85_Datasheet.pdf