

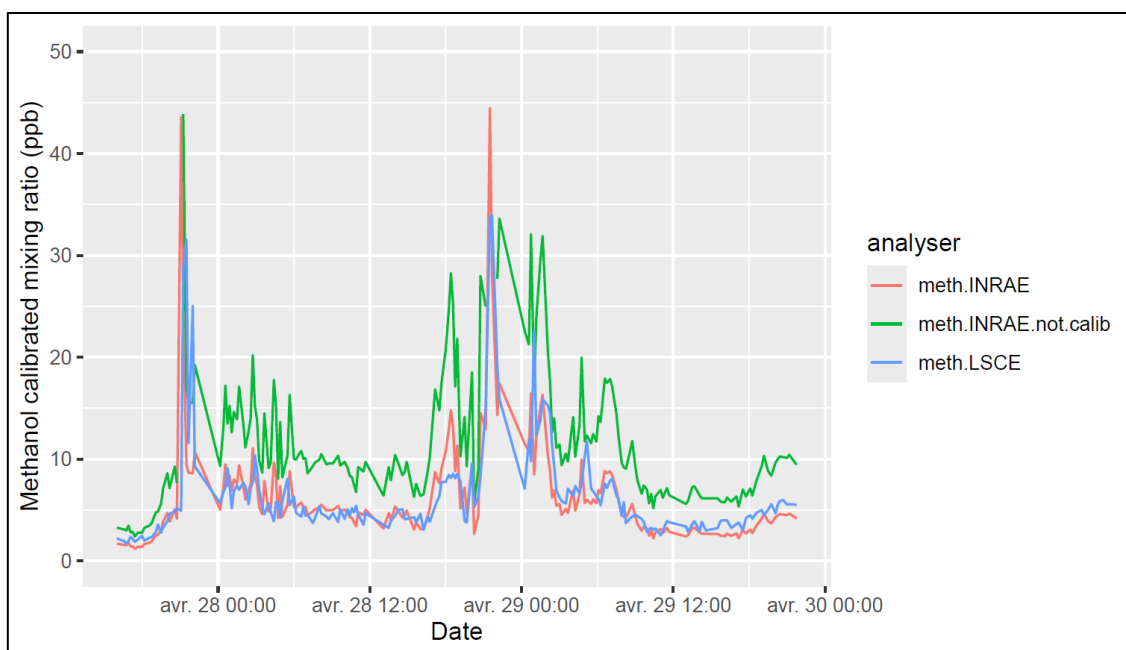


Figure 1 Comparison of methanol mixing ratio measured by the calibrated PTR-HR-MS from the LSCE team (meth.LSCE), by the PTRQI-TOF-MS from the INRAE team as obtained with the calibration procedure (meth.INRAE.not.calib), and after post-calibration against the LSCE PTRMS (meth.INRAE).