

# Technical Note: Using DEG CPCs at upper tropospheric temperatures

**D. Wimmer<sup>1,2</sup>, K. Lehtipalo<sup>2,3</sup>, T. Nieminen<sup>2,4</sup>, J. Duplissy<sup>2,4</sup>, S. Ehrhart<sup>1,5</sup>, J. Almeida<sup>1,5</sup>, L. Rondo<sup>1</sup>, A. Franchin<sup>2</sup>, F. Kreissl<sup>1</sup>, F. Bianchi<sup>6, 7</sup>, H. E. Manninen<sup>2</sup>, M. Kulmala<sup>2</sup>, J. Curtius<sup>1</sup>, and T. Petäjä<sup>2</sup>**

<sup>1</sup>Institute for Atmospheric and Environmental Sciences, Goethe-University of Frankfurt, 60438 Frankfurt am Main, Germany

<sup>2</sup>Department of Physics, University of Helsinki, FI-00014 Helsinki, Finland

<sup>3</sup>Airmodus Ltd, Helsinki, Finland

<sup>4</sup>Helsinki Institute of Physics, FI-00014, Helsinki, Finland

<sup>5</sup>CERN, CH-1211 Geneva, Switzerland

<sup>6</sup>Laboratory for Atmospheric Chemistry, Paul Scherrer Institute, 5232 Villigen, Switzerland

<sup>7</sup>Institute for Atmospheric and Climate Science, ETH Zürich, 8092 Zürich, Switzerland

Correspondence to: D. Wimmer  
([daniela.wimmer@helsinki.fi](mailto:daniela.wimmer@helsinki.fi))

## Abstract

Over the last few years, several Condensation Particle Counters (CPC) capable of measuring in the sub-3 nm size range have been developed. Here we study the performance of diethylene glycol (DEG) based CPCs at different temperatures during Cosmics Leaving OUtdoor Droplets (CLOUD) measurements at CERN. The data shown here is the first set of verification measurements for sub-3 nm CPCs under upper tropospheric temperatures using atmospherically relevant aerosol particles. To put the results in perspective we calibrated the DEG-CPC at room temperature, resulting in a cut-off diameter of 1.4 nm. All diameters refer to mobility equivalent diameters in this manuscript. At upper tropospheric temperatures ranging from 246.15 K to 207.15 K, we found cut-off sizes relative to a PSM in the range of 2.5 to 2.8 nm. Due to low number concentration after size classification, the cut-off diameters have a high uncertainty ( $\pm 0.3$  nm) associated with them. Operating two laminar flow DEG CPCs with different cut-off sizes together with other aerosol instruments, we looked at the growth rates of aerosol population in the CLOUD chamber for particles smaller than 10 nm at different temperatures. A more consistent picture emerged when we normalized the growth rates to a fixed gas-phase sulfuric acid concentration. All of the instruments detected larger growth rates at lower temperatures, and the observed growth rates decreased as a function of temperature, showing a similar trend for all instruments. The theoretical calculations had a similar, but much smaller temperature dependency.

## 1 Introduction

Condensation particle counters (CPCs) measure the total number concentration of aerosol particles by activating and growing them with a supersaturated vapour. Once the particles are grown they are counted optically with a laser (McMurry, 2000). CPCs provide information about the total particle concentration above a certain size. The parameter used to describe the performance of a CPC is the cut-off diameter, which is defined as the diameter at which the particles are counted with 50% efficiency. By using several CPCs with different cut-off diameters, addi-

tional information such as the growth rates can be retrieved (Riipinen et al., 2007; Riccobono et al., 2012; Lehtipalo et al., 2014). In this paper all diameters refer to mobility equivalent diameters (Mäkelä et al., 1996). CPCs capable of measuring reliably in the size range below 3 nm have been developed only recently (Kuang et al., 2012a,b; Vanhanen et al., 2011; Sipilä et al., 2009). The work presented here, focuses on ultrafine CPCs using diethylene glycol (DEG) as condensing liquid, which has been tested in a study by Iida et al. 2009 and proven to be suited for activation of sub-3 nm aerosol particles. CPCs are widely used for ground-based measurements, but they are also deployed during airborne measurements (Crumeyrolle et al., 2010; O'Dowd et al., 1998; Schobesberger et al., 2013), where ambient conditions, such as temperature and pressure, are changing. It has been shown (Kulmala et al., 2007; Wimmer et al., 2013; Kangasluoma et al., 2014) that the counting efficiency curves of the sub-3nm CPCs change according to the particle composition. As the working principle of laminar flow CPCs is based on creating supersaturation and activation by creating a temperature difference, their performance might depend also on the ambient temperature. One issue with CPCs measuring at low temperatures is whether the particles evaporate during the transition from the cold measurement environment to the warmer CPC. Another issue is whether the temperature profile (and thus supersaturation) inside the instrument changes when cold sample air is brought in, possibly resulting in a cut-off shift.

At CLOUD5, which took place in fall 2011 at CERN, measurements were performed to study nucleation under upper tropospheric temperatures. The potential influence of the ambient temperature on the detection efficiency of the CPC used for determining the nucleation rates at 2 nm was investigated. It has been shown that growth rates can be size dependent (Kulmala et al., 2013; Nieminen et al., 2010), especially in the smaller sizes, resulting in a need to determine them reliably. Growth rates were determined at 2 nm using different instruments. The comparison with an ion spectrometer gives important additional information, as the effects of the sample air temperature on the particle detection method, such as volumetric flow rate and mobility to diameter conversion can be accounted for.

The aim of this study is to investigate the possibility to use CPCs at temperatures, which

can be encountered in the upper troposphere (UT; e.g. during flight measurements). Note that the experiments presented here were carried out at ambient pressure plus 4-5 mbar over-pressure. Therefore, influences of operating the CPCs at UT pressures on the cut-offs and other performance characteristics of the CPCs were not investigated in our study. The chamber is operated at this slight over-pressure to avoid accidental contamination. We studied how the counting efficiency curve of a laminar flow DEG CPC changes when varying the temperature and how the sub-3 nm growth rates behave at low temperatures by using different instruments.

## 2 The CLOUD facility

The CLOUD experiment was designed to study nucleation in a controlled environment under well-defined conditions, such as trace gas composition, relative humidity, temperature, etc (Duplissy et al., 2010; Kirkby et al., 2011). In the design, great care was taken to ensure high cleanliness, as it has been shown that impurities of trace gases (already at concentrations as low as few ppt<sub>v</sub>), such as NH<sub>3</sub> influence the nucleation rates (Ball et al., 1999; Kirkby et al., 2011; Schobesberger et al., 2013). The chamber as well as all the gas lines and connections to the chamber are made of stainless steel. The CLOUD facility comprises a 26.1 m<sup>3</sup> cylindrical stainless steel chamber equipped with a fibre optic UV system (Kupc et al., 2011). It includes a very stable temperature control unit ( $\pm 0.01$  K) with a temperature range from 203.15 K up to 373.15 K. Two mixing fans are installed in the upper and lower part of the chamber to ensure homogenous internal mixing (Voigtländer et al., 2012). Measurements can be performed under high ion pair production rates (pion beam from CERN proton-synchrotron on, clearing field grounded), natural level of ion production rates (beam off, clearing field grounded) and completely neutral conditions (beam off, clearing field on). The clearing field is created by applying  $\pm 30$  kV to two circular grids at the top and the bottom of the chamber, removing the small ions, which are continuously generated by the galactic cosmic rays, in less than 1 s. The nucleation measurements in the CLOUD5 campaign, which took place in fall 2011, were mainly performed at three different temperature ranges: between [206-208] K, [221-223] K and [245-248] K. To compare the performance of the chamber and the instruments to previous ex-

periments, measurements at 278.15 K were also performed. In CLOUD the instruments draw air from sampling lines with a length of 75 cm and an outer diameter of 1/2 or 1 inch depending on the required sample flow rate. The chamber is operated under over-pressure of 4-5 mbar. Under-pressure is to be avoided, as ambient air, DEG or butanol vapors from the instruments could leak back into the chamber, for example during a pump failure. To guarantee the same temperature in the chamber and in the sampling lines, the sampling lines were thermally coupled to the chamber, using copper. To avoid thermal exchange with the room air, the sampling lines were wrapped with thermal insulation material on top of the copper wires.

For the measurements analyzed in this study, the particles formed in the CLOUD chamber, consisted mainly of sulfuric acid and water. A Chemical Ionisation Mass Spectrometer (CIMS, (Kürten et al., 2011)) was used for measuring the gaseous sulfuric acid (SA) concentration. The sub-5nm CPCs that were used for measuring the total particle concentrations and calculating nucleation and growth rates were a Particle Size Magnifier (PSM; Airmodus A09), a butanol based laminar flow CPC (3776; TSI Inc.) and two DEG based laminar flow CPCs. Details about the setup and performance of the DEG CPCs can be found in Wimmer et al., 2013. In short, the DEG-CPC1 was set to a saturator temperature of 325 K and an inlet flow rate of 1.5 lpm, whereas the DEG-CPC 2 has a saturator temperature of 328 K and an inlet flow rate of 1.8 lpm. The condenser temperatures are 283 K in both cases. It should be noted that the Differential Mobility Analyzer (DMA) that was used for size selecting the particles for the calibration measurements shown here was a commercial nano-DMA (nano-DMA; Grimm Aerosol Technik, S-DMA, 55-100), whereas for the calibration measurements at room temperature, a high-resolution DMA (Herrmann et al., 2000) was used, resulting in a better size resolution for those measurements. A comparison of the performance of the different DMAs can be found in Jiang et al., 2011a.

### **3 Calibrating CPCs using the CLOUD chamber as an aerosol source**

The calibration unit consisted of the CLOUD chamber as the particle source. Doing so, the calibration particle composition was exactly the same as during the nucleation experiments. The

particle production was triggered by switching on the UV lamp after adding SO<sub>2</sub>, O<sub>3</sub> and water vapour to the chamber. The particles were sampled from a core sampling probe, which was used to minimize diffusion losses. The core sampling probe consisted of a coaxial tube with a conical tip and an outer diameter of 6 mm. A fraction of the flow was sampled through that tube from the center of the flow, whereas the flow closer to the walls of the main tube was discarded. No external charger was used, only the naturally negatively charged fraction of particles which were size selected with a nano-DMA (Grimm Aerosol Technik, S-DMA, 55-100) were used for the calibration. The laminar flow DEG CPC1 was calibrated according to the setup shown in Figure 1. To measure the total concentration after the DMA, as a first test, a Faraday Cup Electrometer was used as a reference. The particle concentrations after the size selection were low due to many factors, including low ion concentrations (about 400 cm<sup>-3</sup>) (Kirkby et al., 2011), fast particle growth (i.e. particles grow out of the desired size range quickly) and internal losses in the DMA. This resulted in an unacceptably high noise to signal ratio and therefore it was decided to use a PSM at a fixed cut size as the reference instrument instead of an electrometer. The PSM has a significantly lower cut-off size than the laminar flow DEG CPC, a steep counting efficiency curve (d<sub>50</sub>=1.1 nm, d<sub>90</sub>=1.5 nm for ammonium sulphate (Wimmer et al., 2013)) and it is a single particle counter. We assume that the PSM behaves similarly to the laminar flow DEG CPC regarding the ambient temperature. To ensure that the cut-off diameter of the PSM stays the same despite varying experimental temperatures, the saturator temperature of the PSM was adjusted for each temperature in the CLOUD chamber. By keeping the homogeneous background in the PSM constant, the assumption is made that the supersaturation within the instrument stays consistent. More detailed discussion about the influence of the temperature settings on the instrument behaviour when using an ultrafine DEG-based CPC can be found in e.g. (Jiang et al., 2011a; Kangasluoma et al., 2015). These assumptions have not been quantified and certainly add some uncertainty to the results. It would be highly interesting to investigate the effect of the ambient temperature on ultrafine CPCs further, but this is not in the scope of this technical note. With this setup, the problem with a too low signal to noise ratio could be reduced and in frame of the measurements presented here, were the best results we could achieve.

During the calibration measurements, the nano-DMA was set to stepping mode, resulting in better statistics for each size bin. The size range of the nano-DMA was limited to a maximum size of 10 nm, which requires to keep the particles in that size range for the time period of each calibration experiment. Slow enough growth was achieved by periodically switching on and off UV lights at very low intensities for a few minutes. As soon as the particles grew to sizes bigger than 10 nm, the UV was switched on again to trigger new formation and growth of small particles. To ensure stable temperature of the calibration system, the DMA was located in a temperature controlled rack, which was kept at 243.15 K for the measurements at 207.25 K and 222.65 K in the chamber, whereas the rack was at 275.15 K for the measurements at 246.25 K in the chamber. Due to technical limitations of the temperature control of the racks and the heat load of the instruments inside the racks, it was impossible to reach the same temperature as in the chamber. For the inlet system to the DMA, a core sampling line was used to lower diffusion losses. The transport flow for the DMA was set to 10 lpm, while the aerosol flow through the DMA was 2 lpm. The sheath flow of the DMA passed through a heat exchanger. The dilution flow after the DMA was taken from a different sampling line to guarantee the same composition and temperature of the stream. By setting the sheath flow to 17 lpm, a good sheath air to sample flow rate ratio was achieved to ensure a narrow size distribution in the DMA (Jiang et al., 2011a).

#### **4 Method for determining growth rates from the DEG CPCs**

The low cut-off CPCs (DEG-CPCs and PSMs) have been used at CLOUD to determine the initial growth rate (GR) of the particles. This is relevant e.g. for scaling the nucleation rates, measured at larger sizes (Kirkby et al., 2011; Almeida et al., 2013; Kulmala et al., 2013) down to smaller sizes (e.g. 1.7 nm)(Kerminen and Kulmala, 2002). To determine whether the shift in the cut-off curves influences the scientific outcome of the measurements with the laminar flow DEG CPCs significantly, the growth rates have been determined and compared to other instruments (NAIS (Mirme and Mirme, 2013) and PSM). The growth rates from the PSM were determined by using two PSMs at different cut sizes together with the other ultrafine CPCs,

according to the method shown in Lehtipalo et al., 2014. From the NAIS the growth rates were determined by following the time-evolution of the maximum concentration in each size-bin of the instrument (Kulmala et al., 2012).

5 An example that illustrates the chosen method for calculating the growth rates is shown in Figure 2. The raw signal from the CPCs was smoothed using a running average of 5 seconds. The total measured number concentration was normalized to the maximum for each run separately. Next, the times when the concentrations reached half of the maximum concentrations were determined. The half maximum is defined by the range between 50 and 60% of the maxi-  
10 mum concentration as even the averaged data shows fluctuations. The time difference between the half maxima of the two DEG CPCs was then used for determining the growth rates. A similar method for establishing GRs from CPCs with different cut-off sizes is described in Riccobono et al., 2012 and Lehtipalo et al., 2014. The cut size of the DEG CPC 2 could not be determined via calibration measurements using the CLOUD chamber. The cut-off diameter was  
15 estimated to be 0.3 nm smaller than the DEG CPC 1, based on the growth rates calculated using different ultrafine CPCs and their respective cut-off diameters (PSM  $d_{50}=1.1$  nm, TSI 3776  $d_{50}=2.9$  nm).

The times used for the growth rate analysis are marked with arrows in Figure 2. The half  
20 maximum points (60% in this case, which was the allowed range due to statistics) here were reached at 14:10:45 and 14:12:50 resulting in a time difference of 125 s and therefore in a GR of 9.3 nm/h. The temperature in the chamber in this case was 223.15 K and the electrodes of the high voltage control were set to  $\pm 30$  kV, so it was a neutral run.

The nucleation experiments in CLOUD which were used for the GR calculations shown here,  
25 were done at different temperatures and sulfuric acid concentrations. To determine a possible temperature trend for the different instruments, the growth rates shown here were normalized to the same sulfuric acid concentration ( $10^7$  cm $^{-3}$ ). This was done by multiplying the calculated growth rates, which are a function of the sulfuric acid concentration with  $10^7$ . This factor was then dividing the by the measured sulfuric acid concentration. That procedure was applied for



each growth rate/SA concentration pair individually (see Equation 1). This is a very simplified method based on the assumption that there is a linear relationship between the growth rates and the sulfuric acid concentration. From the measurements with a high-resolution mass spectrometer, it is known that at temperatures below 278 K, the major species contributing to the nucleation and growth in the CLOUD chamber, is sulfuric acid (Schobesberger et al., 2013). The normalization was done using the following equation

$$GR_{norm} = GR_{calc}(\text{H}_2\text{SO}_4) * 10^7 / \text{H}_2\text{SO}_{4\text{meas}}, \quad (1)$$

$GR_{calc}$  here means the GRs calculated from the CPC measurements and  $\text{H}_2\text{SO}_{4\text{meas}}$  means the measured sulfuric acid concentration from the CIMS. Growth rates higher than 20 nm/h have been neglected, as then the time difference between the two laminar flow DEG CPCs becomes too small.

## 5 Results

### 5.1 Upper tropospheric temperature calibration results

Figure 3 shows the calibration curves at different temperatures (207.25 K, 222.65 K, 246.25 K, 293 K). Due to the huge scatter and large error bars a number of the red data points seem to indicate a small cut-off at 208.15 K, but the majority of the data points below 2 nm is at zero and the fit shows that the cut-off relative to a PSM is shifted. The data points in Figure 3 are taken from the experiments with the highest particle concentrations after the DMA. Three-parameter sigmoidal fits (Stolzenburg and McMurry, 1991) are applied to the measured data points

$$\text{fit}(d_p) = a + b / (1 + \exp(-c \cdot (d_p - d_{50}))), \quad (2)$$

and are weighted based on the error bars of the measured data points. To fit the 207.25 K data, the parameter  $c$  (= rate of change in 1/nm) had to be fixed to 0.3 and also the base value (parameter  $a$ ) was fixed to 0, otherwise the fit would not have converged due to the large error bars in the smaller sizes. The values for the half maxima (=  $d_{50}$ ) given by the fits are  $2.5 \pm 0.05$  for

the data points at 207.25 K,  $(2.6 \pm 0.1)$  nm for 246.25 K and  $(2.8 \pm 0.05)$  nm for the data taken at 222.65 K. As the overall particle concentration after the DMA was typically  $10 \text{ cm}^{-3}$ , the relative errors of the measurements are large. This means that the results are qualitative. Time and technical limitations prevented the acquisition of more data.

5

Nevertheless there is a clear shift in the cut-off diameter relative to a PSM, towards larger sizes at lower temperatures. Analysis, using CLOUD5 run data at higher temperatures for determining the cut-offs of the DEG-CPCs at room temperature (295 K) showed comparable results to the laboratory calibration measurements ( $d_{50} \sim 1$  nm). The shift in the cut-off size from room  
10 temperature to UT temperatures could be caused by shifts in the internal temperature-dependent diffusion losses. The calculation (Baron and Willeke, 2001) shows that this difference is negligible. At 246.25 K, the diffusion loss corrected  $d_{50}$  is at 2.7 nm, whereas it is 2.8 nm for the uncorrected data. It is worth noting here that the temperature controlled rack was set to the same temperature (243 K) for the calibration measurements at 207 and 222 K. The calibrations at a  
15 chamber temperature of 246.25 K were done with a rack temperature of 243 K, which is much closer to the chamber temperature.

Two effects could cause the shift in the counting efficiency curves. The first one, is a possible change in the profile of supersaturation in the condenser of the CPC, due to a different tempera-  
20 ture of the sample flow. In that case, the shift would be expected to be a function of temperature. Modelling results, using COMSOL 5.0 multiphysics model show that assuming a constant flow of 0.3 lpm from the inlet of the CPC until the beginning of the capillary, the final temperature of the flow is 326 K for an inlet temperature of 208.15 K and the same for an inlet temperature of 298.15 K. The dimensions that were used for the modelling are: 2.2 cm inlet at ambient  
25 temperature, 17.3 cm inside the CPC cabin, assuming at temperature of 303.15 K and 2.7 cm inside the saturated region, assuming a temperature of 328.15 K. These results suggest that the ambient temperature does not influence the profile of the saturation ratio in the condenser of the CPC. The second effect would be that the shift is caused by evaporation of particles before being activated in the CPC. This means that, after the particles are size-selected in the DMA,

which is still in the cold environment, they shrink. That leads to a shift in the counting efficiency as the particles changed in size after they were size selected.

## 5.2 Comparison of growth rates

Figure 4 shows the growth rates normalized to a  $\text{H}_2\text{SO}_4$  concentration of  $10^7 \text{ cm}^{-3}$  (Equation 1) in nm/h on the y-axis as a function of temperature for the laminar flow DEG CPCs, the PSMs and the NAIS. All the GRs are determined at about 2 nm. The normalized GRs are averaged for the different temperature ranges [206-208] K, [221-223] K and [245-248] K and also the temperatures are averaged for each range. The error bars show the standard deviation of the averages of the growth rates. The growth rates are higher for lower temperatures and the growth rates decrease with increasing temperature, showing the same trend for all the instruments. The GR calculated from the DEG CPCs and the PSM agree within a factor of 1.2, whereas the GR from the NAIS are about a factor of 2.2 higher compared to the DEG CPCs at 208.15 K. The higher GR from the NAIS might be due to the fact that it was measuring negatively charged particles only which are expected to be higher than neutral GRs (Laakso et al., 2003). They were calculated following the maximum concentration in each size bin of the NAIS (Kulmala et al., 2012). The growth rates due to kinetic collision limited condensation of sulphuric acid show the opposite trend, i.e. slight increase of the growth rate as function of temperature (Nieminen et al., 2010). This is very likely due to the effect that this calculation does not take evaporation from the particles into account.

## 5.3 Theoretical calculation of growth rates

The GR can be described as,

$$GR = k_c \Delta d_p, \quad (3)$$

$\Delta d_p$  is the change of diameter due to the condensing sulfuric acid and  $k_c$  is the condensation rate. The condensation rate and the change in diameter was determined for a particle of 2 nm with the SAWNUC model (Lovejoy et al., 2004). Equation 3 is only valid for situations without

evaporation. Very small particles have higher evaporation rates than bigger particles, due to the Kelvin effect (Mckenzie et al., 1984). In fact particles below the critical diameter, if such a diameter exists, will mainly evaporate while particles bigger than the critical diameter will grow. In these calculations the evaporation effect on the growth rate is given by,

$$GR = (k_c - k_e) \Delta d_p. \quad (4)$$

With  $k_e$  being the evaporation rate as described by Lovejoy et al., 2004. This equation accounts for the evaporation of particles. The relative contribution of evaporation versus condensation, is determined by the vapour pressure of the condensing species. At higher temperatures the growth rates were calculated for a sulfuric acid concentration of  $7 \cdot 10^8 \text{ cm}^{-3}$ , as at this temperature a significant background contamination of  $\text{NH}_3$  was present in the CLOUD chamber (Kirkby et al., 2011).  $\text{NH}_3$  can lower the saturation vapour pressure of sulfuric acid over these small aerosols, though the magnitude of this effect depends on the composition in gas and aerosol phase (Clegg et al., 2008). SAWNUC includes only aerosols containing  $\text{H}_2\text{SO}_4$  and water in the calculation, the calculations give nevertheless a good indication about the growth rate behaviour when evaporation can not be neglected. The results from those calculations compared to the experimental data are shown as the purple triangles in Figure 4. The comparison with the data shows that the SAWNUC predictions show a similar temperature trend as the experimental data (i. e. smaller GR above  $0^\circ\text{C}$ ). This drop off at higher temperatures remains unclear, nevertheless the higher GR retrieved from the NAIS data compared to the SAWNUC model and to the GRs from the CPCs at the lower temperatures might be due to a charge enhancement (Laakso et al., 2003).

## 6 Conclusions

We investigated the performance of the Diethylene Glycol (DEG) based CPC under temperatures typical for the upper troposphere, by performing a set of calibration measurements at temperatures between 248.15 K and 208.15 K. Here the CLOUD chamber was used as aerosol particle source and a nano-DMA to size select the particles. As the total particle concentra-

tion was low, a single particle counter (Particle Size Magnifier; PSM) was used as reference instrument for the calibration measurements. The results show that there is a shift in the cut-off diameter of the CPC towards bigger sizes compared to the laboratory calibrations at room temperature. The cut-off sizes, relative to a PSM, were 2.5 nm for 207.25 K, 2.8 nm for 222.65 K, 2.6 nm for 246.25 K and 1.4 nm relative to an electrometer, for 298.15 K (room temperature) for the DEG CPC1. As the maximum concentration of particles after the DMA was about  $10\text{ cm}^{-3}$ , the uncertainty in the cut-off diameters retrieved from those measurements are large. This means that the results show a clear shift in the cut-off diameters towards the bigger sizes, but the exact numbers for the cut-off diameters need to be treated carefully. Despite the big uncertainties in the measurement results, for the first time, a sub-3 nm CPC has been calibrated under upper tropospheric relevant temperatures. In addition the calibration measurements were done using the same particle composition as for the nucleation measurements.

We used a method to analyze growth rates based on the difference in the cut-off sizes between two DEG CPCs, using the results from the calibration measurements and compared the calculated growth rates with those derived from other instruments. To evaluate the validity of the results, the GR have been compared to the growth rates determined from mixing type CPCs (PSMs) and an ion spectrometer (NAIS) at different temperatures. All the instruments show higher GRs for lower temperatures. The average value of the growth rates from the NAIS show somewhat higher values (factor of 2.2) compared to the GRs determined from the DEG CPCs. The growth rates derived from the PSM and DEG CPCs agree within a factor of 1.2. The growth rates show a similar temperature trend for all instruments and theoretical calculations. This indicates that growth rates at low temperatures might be under-estimated. However the CPCs detect both charged and neutral particles, whereas the NAIS measured charged particles. The GRs calculated from kinetically limited collision rates of sulfuric acid and water show the opposite temperature trend, but here evaporation is not taken into account. The SAWNUC (Lovejoy et al., 2004) model where evaporation is taken into account, shows a similar temperature trend as the experimental data.

We have shown that when using CPCs at upper tropospheric temperatures, it has to be taken

into account that cut-off diameters might be shifted towards bigger sizes. This effect might be due to evaporation of the smallest particles. We ruled out the possibility of a change of the CPC performance by modelling the temperature profiles if the CPC inlet for 208.15 K and 295.15 K. The modelling results show the exact same resulting temperature at the beginning of the aerosol capillary. That suggests that the effect leading to the shift in the cut-off diameter is due to particle evaporation in the transition from the cold chamber into the warm CPC. Taking the cut-off shift (due to evaporation) into account, CPCs can still be reliably used as total particle counters, depending on the size distribution.

*Acknowledgements.* We would like to thank CERN for supporting CLOUD with important technical and financial resources, and for providing a particle beam from the CERN Proton Synchrotron. We also thank P. Carrie, L.-P. De Menezes, J. Dumollard, F. Josa, I. Krasin, R. Kristic, A. Laassiri, O.S. Maksimov, B. Marichy, H. Martinati, S.V.Mizin, R.Sitals, A.Wasem and M.Wilhelmsson for their important contributions to the experiment. We would like to thank Francesco Riccobono for helping with the setup of the calibration unit and we would also like to thank Jasper Kirkby for giving the opportunity to use the CLOUD chamber for the calibration measurements. This research has received funding from the EC Seventh Framework Programme (Marie Curie Initial Training Network 'CLOUD-ITN' no. 215072, MC-ITN 'CLOUD-TRAIN' no. 316662, ERC-Starting 'MOCAPAF' grant no. 57360 and ERC-Advanced 'ATMNUCLE' grant no. 227463), the German Federal Ministry of Education and Research (project nos.01LK0902A and 01LK1222A), the Swiss National Science Foundation (project nos. 200020 135307 and 206620 130527), the Academy of Finland (Center of Excellence project no. 1118615), the Academy of Finland (135054, 133872, 251427, 139656, 139995, 137749, 141217, 141451), the Finnish Funding Agency for Technology and Innovation, the Väisälä Foundation, the Nessling Foundation, the Austrian Science Fund (FWF; project no. P19546 and L593), the Portuguese Foundation for Science and Technology (project no. CERN/FP/116387/2010), the Swedish Research Council, Vetenskapsrådet (grant 2011-5120), the Presidium of the Russian Academy of Sciences and Russian Foundation for Basic Research (grants 08-02-91006-CERN and 12-02-91522-CERN), and the U.S. National Science Foundation (grants AGS1136479 and CHE1012293).

## References

- Almeida, J., Schobesberger, S., Kürten, A., Ortega, I. K., Kupiainen, O., Praplan, A. P., Amorim, A., Bianchi, F., Breitenlechner, M., David, A., Dommen, J., Donahue, N. M., Downard, A., Dunne, E., Duplissy, J., Ehrhart, S., Flagan, R. C., Franchin, A., Roberto, G., Hakala, J., Hansel, A., Heinritzi, M.,  
5 Jokinen, T., Junninen, H., Kajos, M. K., Keskinen, H., Kupc, A., 'en, T. K., Kvashin, A., Laaksonen, A., Lehtipalo, K., Leiminger, M., Leppä, J., Loukonen, V., Makhmutov, V., Mathot, S., McGrath, M., Nieminen, T., Olenius, T., Onnela, A., Petäjä, T., Riccobono, F., Riipinen, I., Rondo, L., Ruuskanen, T., Santos, F. D., Schallhart, S., Schnitzhofer, R., Seinfeld, J. H., Simon, M., Sipilä, M., Stozhkov, Y., Stratmann, F., Tomé, A., Tröstl, J., Tsagkogeorgas, G., Vaattovaara, P., Viisanen, Y., Virtanen, A.,  
10 Vrtala, A., Wagner, P., Weingartner, E., Wex, H., Williamson, C., Wimmer, D., Ye, P., Yli-Juuti, T., Carslaw, K., Kulmala, M., Curtius, J., Baltensperger, U., Worsnop, D., Vehkamäki, H., and Kirkby, J.: Molecular understanding of amine-sulphuric acid particle nucleation in the atmosphere, *Nature*, 502, 2013.
- Ball, S. M., Hanson, D. R., Eisele, F. L., and McMurry, P. H.: Laboratory studies of particle nucleation:  
15 Initial results for H<sub>2</sub>SO<sub>4</sub>, H<sub>2</sub>O and NH<sub>3</sub> vapors, *J. Geophys. Res. - Atmospheres*, 104, 23,709–23,718, 1999.
- Clegg, S., Kleemann, M. J., Griffin, R. J., and Seinfeld, J. H.: *Atmos. Chem. Phys.*, 8, 2008.
- Crumeyrolle, S., Manninen, H. E., Sellegri, K., Roberts, G., Gomes, L., Kulmala, M., Weigel, R., Laj, P., and Schwarzenböck, A.: New particle formation events measured on board the ATR-42 aircraft  
20 during the EUCAARI campaign, *Atmos. Chem. Phys.*, 10, 6721–6735, 2010.
- Duplissy, J., Enghoff, M. B., Aplin, K. L., Arnold, F., Aufmhoff, H., Avngaard, M., Baltensperger, U., Bondo, T., Bingham, R., Carslaw, K., Curtius, J., David, A., Fastrup, B., Gagné, S., Hahn, F., Harrison, R. G., Kellet, B., Kirkby, J., Kulmala, M., Laakso, L., Laaksonen, A., Lillestol, E., Lockwood, M., Mäkelä, J., Makhmutov, V., Marsh, N. D., Nieminen, T., Onnela, A., Pedersen, E., Pedersen, J.  
25 O. P., Polny, J., Reichl, U., Seinfeld, J. H., Sipilä, M., Stozhkov, Y., Stratmann, F., Svensmark, H., Svensmark, J., Verheggen, B., Viisanen, Y., Wagner, P. E., Wehrle, G., Weingartner, E., Wex, H., Wilhelmsson, M., and Winkler, P. M.: Results from the CERN pilot CLOUD experiments, *Atmos. Chem. Phys.*, 10, 1635–1647, 2010.
- Herrmann, W., Eichler, T., Bernardo, N., and Fernandez de la Mora, J.: Turbulent Transition Arises at  
30 Reynolds Number 35,000 in a Short Vienna Type DMA with a Large Laminarization Inlet, in: AAAR, annual conference, St Louis, Minnesota, USA, 2000.
- Iida, K., Stolzenburg, M. R., and McMurry, P. H.: Effect of Working Fluid on Sub-2 nm Particle Detec-

tion with a Laminar Flow Ultrafine Condensation Particle Counter, *Aerosol Sci. Technol.*, 43, 81–96, 2009.

Jiang, J., Attoui, M., Heim, M., Brunelli, N. A., McMurry, P. H., Kasper, G., Flagan, R. C., Giapis, K., and Mouret, G.: Transfer Functions and Penetrations of Five Differential Mobility Analyzers for Sub-2 nm Particle Classification, *Aerosol Sci. Technol.*, 45, 480–492, 2011a.

Jiang, J., Chen, M., Kuang, C., Attoui, M., and McMurry, P. H.: Electrical Mobility Spectrometer Using a Diethylene Glycol Condensation Particle Counter for Measurement of Aerosol Size Distributions Down to 1 nm, *Aerosol Sci. Technol.*, 45, 510–521, 2011b.

Kangasluoma, J., Kuang, C., Wimmer, D., Rissanen, M. P., Lehtipalo, K., Ehn, M., Worsnop, D. R., Wang, J., Kulmala, M., and Petäjä, T.: Sub-3nm particle size and composition dependent response of a nano-CPC battery, *Atmos. Meas. Tech.*, 7, 689–700, 2014.

Kangasluoma, J., Franchin, A., Duplissy, J., Ahonen, L., Korhonen, F., Attoui, M., Mikkilä, J., Lehtipalo, K., Vanhanen, J., Kulmala, M., and Petäjä, T.: Operation of the Airmodus A11 nano Condensation Nucleus Counter at different inlet pressures, different operation temperatures and design of a new inlet system, submitted to *Atmos. Meas. Tech. Discuss.*, 2015.

Kerminen, V.-M. and Kulmala, M.: Analytical formulae connecting the 'real' and the 'apparent' nucleation rate and the nuclei number Concentration for atmospheric nucleation events, *J. Aerosol Sci.*, 33, 609–622, 2002.

Kirkby, J., Curtius, J., Almeida, J., Dunne, E., Duplissy, J., Ehrhart, S., Franchin, A., Gagné, S., Ickes, L., Kürten, A., Kupc, A., Metzger, A., Riccobono, F., Rondo, L., Schobesberger, S., Tsagkogeorgas, G., Wimmer, D., Amorim, A., Bianchi, F., Breitenlechner, M., David, A., Dommen, J., Downard, A., Ehn, M., Flagan, R. C., Haider, S., Hansel, A., Hauser, D., Jud, W., Junninen, H., Kreissl, F., Kvashin, A., Laaksonen, A., Lehtipalo, K., Lima, J., Lovejoy, E. R., Makhmutov, V., Mathot, S., Mikkilä, J., Minginette, P., Mogo, S., Tuomo, N., Onnela, A., Pereira, P., Petäjä, T., Schnitzhofer, R., Seinfeld, J. H., Sipilä, M., Stozhkov, Y., Stratmann, F., Tomé, A., Vanhanen, J., Viisanen, Y., Vrtala, A., Wagner, P. E., Hansueli, W., Weingartner, E., Wex, H., Winkler, P. M., Carslaw, K. S., Worsnop, D. R., Baltensperger, U., and Kulmala, M.: Role of sulphuric acid, ammonia and galactic cosmic rays in atmospheric aerosol nucleation, *Nature*, 476, 429–433, 2011.

Kuang, C., Chen, M., McMurry, P. H., and Wang, J.: Modification of Laminar Flow Ultrafine Condensation Particle Counters for the enhanced detection of 1 nm condensation nuclei, *Aerosol Sci. Technol.*, 46, 309–315, 2012a.

Kuang, C., Chen, M., Zhao, J., Smith, J., McMurry, P. H., and Wang, J.: First size-dependent growth rate measurements of 1 to 5nm freshly formed atmospheric nuclei, *Atmos. Chem. Phys.*, 12, 3537–3589,



2012b.

- Kulmala, M., Mordas, G., Petäjä, T., Grönholm, T., Aalto, P. P., Vehkamäki, H., Hienola, A. I., Herrmann, E., Sipilä, M., Riipinen, I., Manninen, H. E., Hämeri, K., Stratmann, F., Bilde, M., Winkler, P. M., Birmili, W., and Wagner, P. E.: The condensation particle counter battery (CPCB): A new tool to  
5 investigate the activation properties of nanoparticles, *J. Aerosol Sci.*, 38, 289–304, 2007.
- Kulmala, M., Petäjä, T., Nieminen, T., Sipilä, M., Manninen, H. E., Lehtipalo, K., Maso, M. D., Aalto, P., Junninen, H., Paasonen, P., Riipinen, I., Lehtinen, K. E. J., Laaksonen, A., and Kerminen, V. M.: Measurement of the nucleation of atmospheric aerosol particles, *Nature Protocols*, 7, 1651–1667,  
2012.
- 10 Kulmala, M., Kontkanen, J., Junninen, H., Lehtipalo, K., Manninen, H. E., Nieminen, T., Petäjä, T., Sipilä, M., Schobesberger, S., Rantala, P., Franchin, A., Jokinen, T., Järvinen, E., Äijälä, M., Kangasluoma, J., Hakala, J., Aalto, P. P., Paasonen, P., Mikkilä, J., Vanhanen, J., Aalto, J., Hakola, H., Makkonen, U., Ruuskanen, T., Mauldin, L. R., Duplissy, J., Vehkamäki, H., Bäck, J., Kortelainen, A., Riipinen, I., Kurtén, T., Johnston, M. V., Smith, J. N., Ehn, M., Mentel, T. F., Lehtinen, K. E. J.,  
15 Laaksonen, A., Kerminen, V.-M., and Worsnop, D. R.: Direct Observations of Atmospheric Aerosol Nucleation, *Science*, 339, 943, 2013.
- Kupc, A., Amorim, A., Curtius, J., Danielczok, A., Duplissy, J., Ehrhart, S., Walther, H., Ickes, L., Kirkby, J., Kürten, A., Lima, J. M., Mathot, S., Minginette, P., Onnela, A., Rondo, L., and Wagner, P. E.: A fibre-optic UV system for H<sub>2</sub>SO<sub>4</sub> production in aerosol chambers causing minimal thermal  
20 effects, *J. Aerosol Sci.*, 42, 532–543, 2011.
- Kürten, A., Rondo, L., Ehrhart, S., and Curtius, J.: Performance of a corona ion source for measurement of sulfuric acid by chemical ionization mass spectrometry, *Atmos. Meas. Tech.*, 4, 437–443, 2011.
- Laakso, L., Kulmala, M., and Lehtinen, K. E. J.: Effect of condensation rate enhancement factor on 3-nm (diameter) particle formation in binary ion-induced and homogeneous nucleation, *Journal of  
25 Geophysical Research-Atmospheres*, 108, 4574, doi:10.1029/2003JD003432, 2003.
- Lehtipalo, K., Leppä, J., Kontkanen, J., Kangasluoma, J., Franchin, A., Wimmer, D., Schobesberger, S., Junninen, H., Petäjä, T., Sipilä, M., Mikkilä, J., Vanhanen, J., Worsnop, D. R., and Kulmala, M.: Methods for determining particle size distribution and growth rates between 1–3 nm using the Particle Size Magnifier, *Boreal Environ. Res.*, 19, 215–236, 2014.
- 30 Lovejoy, E. R., Curtius, J., and Froyd, K. D.: Atmospheric ion-induced nucleation of sulfuric acid and water, *J. Geophys. Res. - Atmospheres*, 109, 204, 2004.
- Mäkelä, J., Riihela, M., Ukkonen, A., Jokinen, V., and Keskinen, J.: Comparison of mobility equivalent diameter with Kelvin-Thomson diameter using ion mobility data, *J. Chem. Phys.*, 105, 1562–1571,

1996.

Mckenzie, R. L., Agarwal, J. K., Pohl, F. G., Preining, O., Reischl, G., Szymanski, W., Wagner, P. E., Liu, B. Y. H., and Pui, D. Y. H.: Measurements of Kelvin-Equivalent Size Distributions of Well-Defined Aerosols with Particle Diameters Greater Than 13 Nm, *Aerosol Sci. Technol.*, 3, 107 – 115, ISI:A1984SM89800013, 1984.

McMurry, P. H.: The History of Condensation Nucleus Counters, *Aerosol Sci. Technol.*, 33, 297–322, 2000.

Mirme, S. and Mirme, A.: The mathematical principles and design of the NAIS- a spectrometer for the measurement of cluster ion and nanometer aerosol size distributions, *Atmos. Meas. Tech.*, 6, 1061–1071, 2013.

Nieminen, T., Lehtinen, K. E. J., and Kulmala, M.: Sub-10 nm particle growth by vapor condensation-effects of vapor molecule size and particle thermal speed, *Atmos. Chem. Phys.*, 10, 9773–9779, 2010.

O'Dowd, C., Geever, M., and Hill, M. K.: New particle formation: Nucleation rates and spatial scale in the coastal environment, *Geophys. Res. Lett.*, 25, 1661–1664, doi:10.1029/98GL01005, 1998.

Riccobono, F., Rondo, L., Sipilä, M., Barmet, P., Curtius, J., Dommen, J., Ehn, M., Ehrhart, S., M., K., Kürten, A., Mikkilä, J., Paasonen, P., Petäjä, T., Weingartner, E., and Baltensperger, U.: Contribution of sulfuric acid and oxidized Organic compounds to Particle Formation and growth, *Atmos. Chem. Phys.*, 12, 9427–9439, doi:10.5194/acp-12-9427-2012, 2012.


Riipinen, I., Sihto, S. L., Kulmala, M., Arnold, F., Dal Maso, M., Birmili, W., Saarnio, K., Teinila, K., Kerminen, V.-M., Laaksonen, A., and Lehtinen, K.: *Atmos. Chem. Phys.*, 7, 1899–1914, 2007.

Schobesberger, S., Junninen, H., Bianchi, F., Lönn, G., Ehn, M., Lehtipalo, K., Dommen, J., Ehrhart, S., Ortega, K. I., Franchin, A., Nieminen, T., Riccobono, F., Hutterli, M., Duplissy, J., Almeida, J., Amorim, A., Breitenlechner, M., Downard, A. J., Dunne, E. M., Flagan, R. C., Kajos, M., Kirkby, H. K. J., Kupc, A., Kürten, A., Kurtén, T., Laaksonen, A., Mathot, S., Onnela, A., Praplan, A. P., Rondo, L., Santos, F. D., Schallhart, S., Schnitzhofer, R., Sipilä, M., Tomé, A., Tsagkogeorgas, G., Vehkamäki, H., Wimmer, D., Baltensperger, U., Carslaw, K. S., Curtius, J., Hansel, A., Petäjä, T., Kulmala, M., Donahue, N. M., and Worsnop, D. R.: Molecular understanding of atmospheric particle formation from sulfuric acid and large oxidized organic molecules, *Proc. Natl. Acad. Sci. U. S. A.*, 110, 17223–17228, 2013.


Sipilä, M., Lehtipalo, K., Attoui, M., Neitola, K., Petäjä, T., Aalto, P. P., O'Dowd, C. D., and Kulmala, M.: Laboratory Verification of PH-CPC's Ability to Monitor Atmospheric Sub-3 nm Clusters, *Aerosol Sci. Technol.*, 43, 126–135, 2009.

Stolzenburg, M. R. and McMurry, P. H.: An Ultrafine Aerosol Condensation Nucleus Counter, *Aerosol*


- Sci. Technol., 14, 48–65, 1991.
- Vanhanen, J., Mikkilä, J., Lehtipalo, K., Sipilä, M., Manninen, H. E., Siivola, E., Petäjä, T., and Kulmala, M.: Particle Size Magnifier for Nano-CN Detection, *Aerosol Sci. Technol.*, 45, 533–542, 2011.
- Voigtländer, J., Duplissy, J., Rondo, L., Kürten, A., and Stratmann, F.: Numerical simulations of mixing  
5 conditions and Aerosol dynamics in the CERN CLOUD chamber, *Atmos. Chem. Phys.*, 12, 2205–  
2214, 2012.
- Wimmer, D., Lehtipalo, K., Franchin, A., Kangasluoma, J., Kreissl, F., Kürten, A., Kupc, A., Metzger, A., Mikkilä, J., Petäjä, T., Riccobono, F., Vanhanen, J., Kulmala, M., and Curtius, J.: Performance of diethylene glycol-based particle counters in the sub-3 nm size range, *Atmos. Meas. Tech.*, 6, 2013.

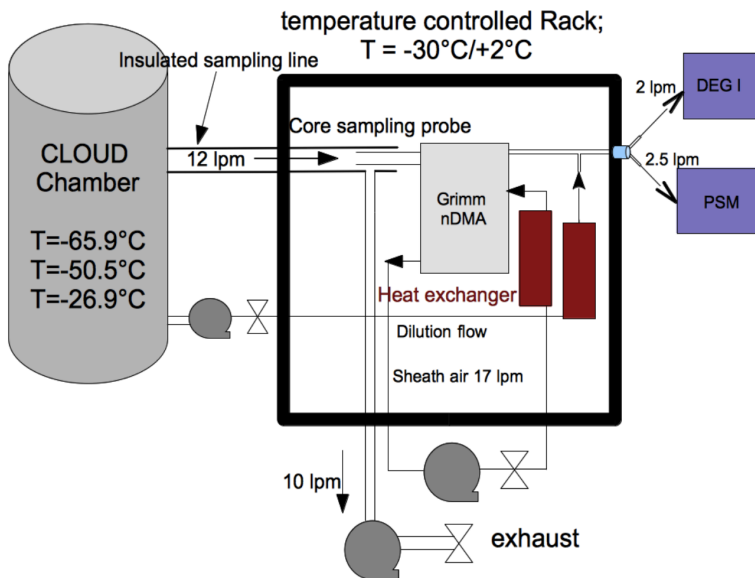


**Fig. 1:** Sketch of the calibration setup. The calibration unit was in a temperature controlled rack, while the CPCs were at room temperature. The temperature inside the rack was 245.15 K for the measurements at lower temperatures, whereas the rack temperature was 275.15 K for the measurements at 246.25 K in the chamber. To minimize diffusion losses, a core sampling probe was used from the chamber to the calibration system. The CLOUD chamber was used to produce naturally charged particles. A nano-DMA was used to size select the particles and as reference a PSM, with a significantly lower cut-off (1.1 nm) than the calibrated CPC. The sheath air of the DMA and the dilution flow after the DMA went through a heat exchanger, consisting of copper tubing to ensure the same temperature for all flows.

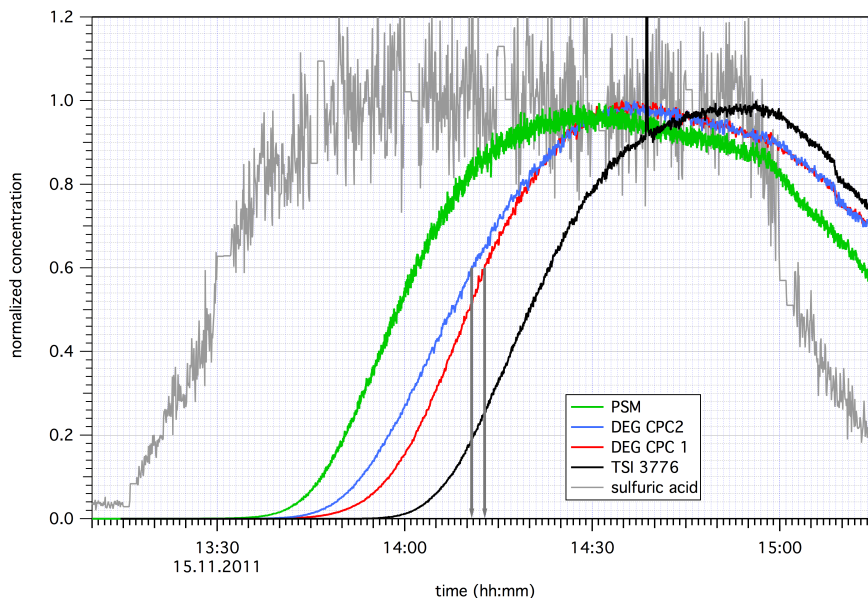

**Fig. 2:** Example of a nucleation experiment during CLOUD5. The temperature inside the chamber in the shown example was 223.15 K and the clearing field was at high voltage, meaning it was a neutral run. The red, blue, green and the black curves show the normalized concentrations for the DEG CPCs, PSM and the TSI 3776 CPC respectively. The grey line shows the normalized sulfuric acid concentration measured by the CIMS. The growth rates are calculated by finding time difference at half maximum between the two DEG CPCs, assuming a difference in diameter of 0.3 nm.

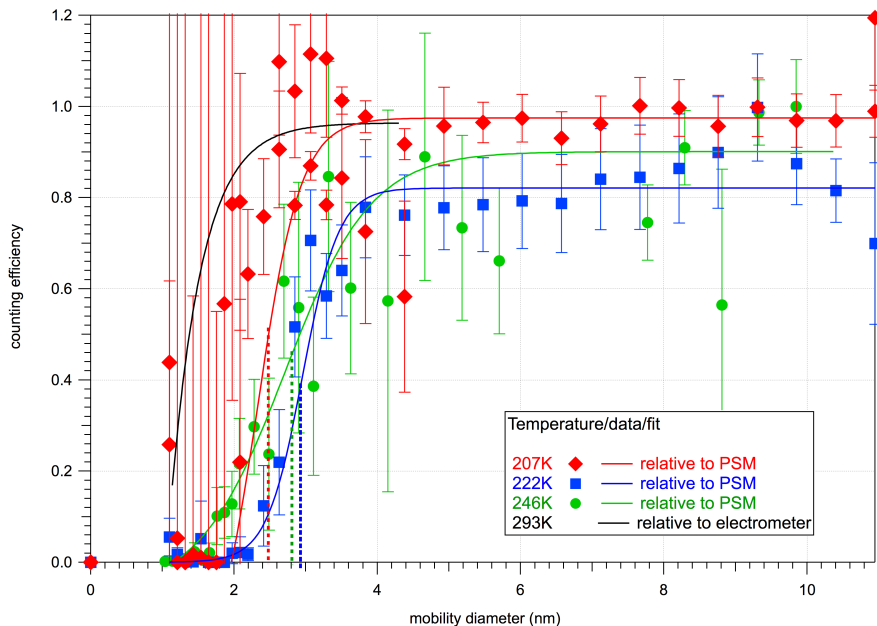

**Fig. 3:** Results from calibration measurements. The blue, green and red curves show fits to the results from calibration measurements for the DEG-CPC1, done at CLOUD in fall 2011 and the symbols show the measured data points, at three different temperatures (246.25 K, 222.65 K, 207.15 K). Black curve shows laboratory calibrations (Wimmer et al., 2013), using negatively charged ammonium sulfate clusters. The  $d_{50}$  relative is shifted from about 1.4 nm at room temperature (relative to an electrometer) to 2.5 nm in the case of 207.15 K about 2.6 nm for 246.25 K and for the 222.65 K, the cut-off is shifted to 2.8 nm. To illustrate the values for the cut-offs, dashed lines pointing to the according sizes are added to the Figure. Due to low statistics, the y-axis error bars are rather large. The error, resulting from the finite width of the transfer function of the nano-DMA, used for the low temperature calibration measurements, is according to Jiang et al., 2011a, 0.185 at 1.47 nm, 0.158 at 1.78 nm and 0.14 at 3 nm.

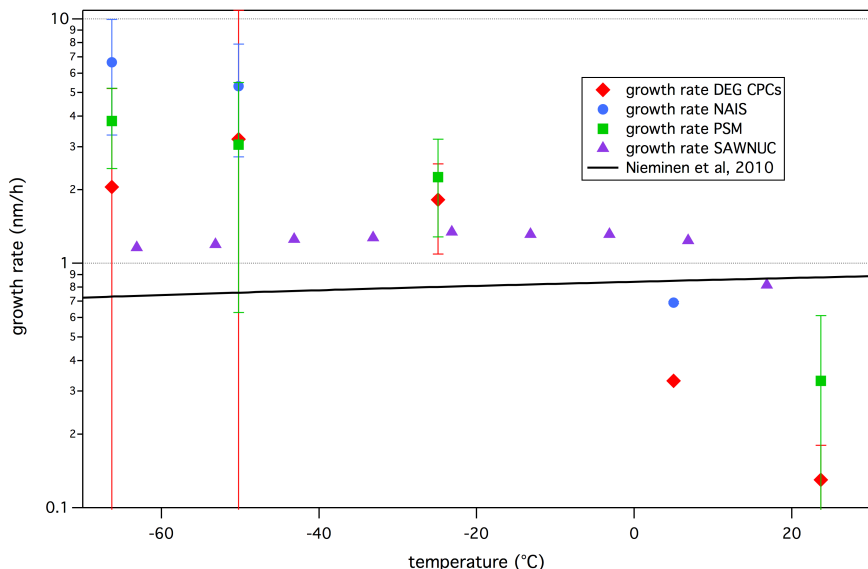

**Fig. 4:** The growth rates normalized to a sulfuric acid concentration of  $10^7 \text{ cm}^{-3}$  as a function of temperature. The GRs have been calculated using the laminar flow DEG CPCs, the PSMs and the NAIS. Red symbols show the average growth rates at the given temperature determined from the DEG CPCs, from the NAIS in blue and from the PSMs in green. The error bars show the standard deviation of the average. The black line shows the expected growth rates based on kinetic collisions of sulfuric acid molecules (Nieminen et al., 2010). The purple triangles show calculations using the SAWNUC model. The modeled results show a similar temperature trend, as here evaporation is taken into account.